






5

**To Set the Decimal Point**




- If it's not already shown, press **MENU** until the unit displays **DEC.P**
- Press **▶/DEV** to show the current decimal point location.
- Press **▲/MAX** to move the decimal point to the desired location. The choices are **FFFF** or **FFF.F**
- Press **MENU** to store the value.



- Press **RESET** twice to display the current temperature.



**To Select Temperature Unit (Fahrenheit or Celsius):**

- Press **MENU** until the display shows **Rd.CF**
- Press **▶/DEV** to display the current temperature unit.
- Press **▲/MAX** to select between °F and °C.



6




- Press **MENU** to store the value.




- Press **RESET** twice to display the current temperature.

**To Enter Setpoints:**

- Press **SETPTS** to display the current setpoint. The leftmost digit will flash.
- Press **▶/DEV** to select the digit you want to change.
- Press **▲/MAX** to increase the value of the flashing digit.




- Press **SETPTS** to store the setpoint.



- Repeat steps 1 through 4 to enter the next setpoint.

**WARNING:** These products are not designed for use in, and should not be used for, patient connected applications.



It is the policy of NEWPORT to comply with all worldwide safety and EMC/EMI regulations that apply. NEWPORT is constantly pursuing certification of its products to the European New Approach Directives. NEWPORT will add the CE mark to every appropriate device upon certification.

The information contained in this document is believed to be correct but NEWPORT Electronics, Inc. accepts no liability for any errors it contains, and reserves the right to alter specifications without notice.

**TRADEMARK NOTICE:**



**Warranty/Disclaimer**

NEWPORT Electronics, Inc. warrants this unit to be free of defects in materials and workmanship for a period of **one (1) year** from the date of purchase. In addition to NEWPORT's standard warranty period, NEWPORT Electronics will extend the warranty period for **four (4) additional years** if the warranty card enclosed with each instrument is returned to NEWPORT.

If the unit malfunctions, it must be returned to the factory for evaluation. NEWPORT's Customer Service Department will issue an Authorized Return (AR) number immediately upon phone or written request. Upon examination by NEWPORT, if the unit is found to be defective, it will be repaired or replaced at no charge. NEWPORT's WARRANTY does not apply to defects resulting from any action of the purchaser, including but not limited to mishandling, improper interfacing, operation outside of design limits, improper repair, or unauthorized modification. This WARRANTY is VOID if the unit shows evidence of having been tampered with or shows evidence of having been damaged as a result of excessive corrosion; or current, heat, moisture or vibration; improper specification; misapplication; misuse or other operating conditions outside of NEWPORT's control. Components which wear are not warranted, including but not limited to contact points, fuses, and triacs.

NEWPORT is pleased to offer suggestions on the use of its various products. However, NEWPORT neither assumes responsibility for any omissions or errors nor assumes liability for any damages that result from the use of its products in accordance with information provided by NEWPORT, either verbal or written. NEWPORT warrants only that the parts manufactured by it will be as specified and free of defects.

NEWPORT MAKES NO OTHER WARRANTIES OR REPRESENTATIONS OF ANY KIND WHATSOEVER, EXPRESS OR IMPLIED, EXCEPT THAT OF TITLE, AND ALL IMPLIED WARRANTIES INCLUDING ANY WARRANTY OF MERCHANTABILITY AND FITNESS FOR A PARTICULAR PURPOSE ARE HEREBY DISCLAIMED.

**LIMITATION OF LIABILITY:** The remedies of purchaser set forth herein are exclusive, and the total liability of NEWPORT with respect to this order, whether based on contract, warranty, negligence, indemnification, strict liability or otherwise, shall not exceed the purchase price of the component upon which liability is based. In no event shall NEWPORT be liable for consequential, incidental or special damages.

**CONDITIONS:** Equipment sold by NEWPORT is not intended to be used, nor shall it be used: (1) as a "Basic Component" under 10 CFR 21 (NRC), used in or with any nuclear installation or activity; or (2) in medical applications or used on humans. Should any Product(s) be used in or with any nuclear installation or activity, medical application, or used on humans, or misused in any way, NEWPORT assumes no responsibility as set forth in our basic WARRANTY/DISCLAIMER language, and, additionally purchaser will indemnify NEWPORT and hold NEWPORT harmless from any liability or damage whatsoever arising out of the use of the Product(s) in such a manner.

**Return Requests/Inquiries**

Direct all warranty and repair requests/inquiries to the NEWPORT Customer Service Department. BEFORE RETURNING ANY PRODUCT(S) TO NEWPORT, PURCHASER MUST OBTAIN AN AUTHORIZED RETURN (AR) NUMBER FROM NEWPORT'S CUSTOMER SERVICE DEPARTMENT (IN ORDER TO AVOID PROCESSING DELAYS). The assigned AR number should then be marked on the outside of the return package and on any correspondence.

The purchaser is responsible for shipping charges, freight, insurance and proper packaging to prevent breakage in transit.

FOR **WARRANTY** RETURNS, please consult NEWPORT for current repair charges. Have the following information available BEFORE contacting NEWPORT:

- P.O. number under which the product was PURCHASED,
- Model and serial number of the product under warranty, and
- Repair instructions and/or specific problems relative to the product.

FOR **NON-WARRANTY** REPAIRS, consult NEWPORT for current repair charges. Have the following information available BEFORE contacting NEWPORT:

- P.O. number to cover the COST of the repair,
- Model and serial number of product, and
- Repair instructions and/or specific problems relative to the product.

NEWPORT's policy is to make running changes, not model changes, whenever an improvement is possible. This affords our customers the latest in technology and engineering.

NEWPORT is a registered trademark of NEWPORT Electronics, Inc.  
© Copyright 2005 NEWPORT Electronics, Inc. All rights reserved. This document may not be copied, photocopied, reproduced, translated, or reduced to any electronic medium or machine-readable form, in whole or in part, without prior written consent of NEWPORT Electronics, Inc.

**PATENT NOTICE:** This product is covered by one or more of the following patents: U.S. Pat. No. Des. 336,895; 5,274,577; 6,243,021 / CANADA 2052599; 2052600 / ITALY 1249456; 1250938 / FRANCE BREVET No. 91 12756 / SPAIN 2039150; 2048066 / UK PATENT No. GB2 249 837; GB2 248 954 / GERMANY DE 41 34398 C2. Other U.S. and International patents pending or applied for.

**QUICK START**



**INFCT and INFCT-xxxB PROGRAMMABLE DIGITAL THERMOCOUPLE CONTROLLER**

For immediate technical or application assistance please call:

**1-800-6397678**  
**1-800-NEWPORT**

Newport Electronics, Inc.  
2229 South Yale Street • Santa Ana, CA • 92704 • U.S.A.  
TEL: (714) 540-4914 • FAX: (203) 968-7311  
Toll Free: 1-800-639-7678 • www.newportUS.com • e-mail: info@newportUS.com  
ISO 9001 Certified

Newport Technologies, Inc.  
976 Bergar • Laval (Quebec) • H7L 5A1 • Canada  
TEL: (514) 335-3183 • FAX: (514) 856-6886  
Toll Free: 1-800-639-7678 • www.newport.ca • e-mail: info@newport.ca

Newport Electronics, Ltd.  
One Omega Drive • River Bend Technology Centre  
Northbank, Irlam • Manchester M44 5BD • United Kingdom  
Tel: +44 161 777 6611 • FAX: +44 161 777 6622  
Toll Free: 0800 488 488 • www.newportuk.co.uk • e-mail: sales@newportuk.co.uk

Newport Electronics spol s.r.o.  
Frystatska 184, 733 01 Karviná • Czech Republic  
TEL: +420 59 6311899 • FAX: +420 59 6311114  
Toll Free: 0800-1-66342 • www.newport.cz • e-mail: info@newport.cz

Newport Electronics GmbH  
Daimlerstrasse 26 • D-75392 Deckenpfronn • Germany  
TEL: 49 7056 9398-0 • FAX: 49 7056 9398-29  
Toll Free: 0800 / 6397678 • www.newport.de • e-mail: sales@newport.de


Mexico and Latin America  
FAX: 001 (203) 359-7807  
En Español: 001 (203) 359-7803


NEWPORTnet™ On-Line Service  
www.newportUS.com  
Internet e-mail  
info@newportUS.com



## Using This Quick Start Manual

Use this Quick Start Manual with your controller to make changes to the thermocouple type, decimal point, units, and to change the setpoints.

Features with  are for the "B" version which has three-color programmable "Big" LED display - All segment characters shown are for the "B" version.


 For detailed instructions, refer to the appropriate section in the Operator's Manual.

## Before You Begin

In addition to the meter and the related parts, you will need the following items to set up your meter:

- ac power, as listed on meter's ID/Power Label
- Thermocouple
- 1/8" flat blade screwdriver

## Safety Consideration

 This device is marked with the international Caution symbol.

The instrument is a panel mount device protected in accordance with EN61010-1 (Safety requirements for electrical equipment for measurement, control, and laboratory standard). Remember that the unit has no power-on switch. Building installation should include a switch or circuit-breaker that must be compliant to IEC 947-1 and 947-3.

### SAFETY:


- Do not exceed voltage rating on the label located on the top of the instrument housing.
- Always disconnect power before changing signal and power connections.
- Do not use this instrument on a work bench without its case for safety reasons.
- Do not operate this instrument in flammable or explosive atmospheres.
- Do not expose this instrument to rain or moisture.

### EMC:


- Whenever EMC is an issue, always use shielded cables.
- Never run signal and power wires in the same conduit.
- Use signal wire connections with twisted-pair cables.
- Install Ferrite Bead(s) on signal wire close to the instrument if EMC problems persist.

## Mount the Unit

- Cut a panel opening using the dimensions shown to the right.
- Position the unit in the opening, making sure the front bezel is flush with the panel.
- Install retaining clip on the meter and tighten against the panel.

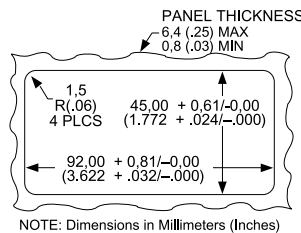


## Wiring


 **Warning: Do not connect AC power to your device until you have completed all input and output connections. This device must only be installed by a specially trained electrician with corresponding qualifications. Failure to follow all instructions and warnings may result in injury!**


- Remove the panel at the back of the unit.
- Locate the TB1 connector.
- Insert the correct wire in each terminal as shown in the following figure and tighten the lockdown screws.
- Tug gently on the wires to verify the connections.

External Fuse Required:  
 Time-delay, UL 248-14 listed 175 mA (115 Vac line)  
 80 mA (230 Vac line)  
 Time-lag, IEC 127-3 recognized 125 mA (115 Vac line)  
 63 mA (230 Vac line)

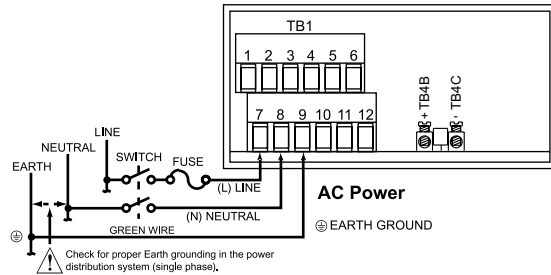


### AC Powered Unit Connections

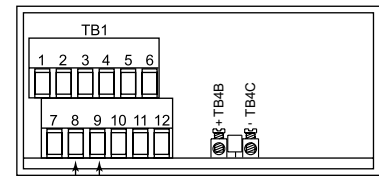

 In order to maintain the same degree of protection as the AC units, always use a Safety Agency Approval DC source with the same Overvoltage Category and Pollution Degree.

### DC Powered Unit Connections

## Wiring the Controller



### Typical Wiring of TB1

## Thermocouple Wire Connection

- Connect positive (+) lead of thermocouple.
- Connect negative (-) lead of thermocouple.

Note: The negative lead is red.

## Example hook up for AC Load

### Alarm 1 (Setpoint) Hook-up

- Connect a jumper from ac Line to Relay 1 Common (Terminal 3).
- Connect Relay 1 Normally Open (Terminal 1) to External Alarm ac Line.
- Connect External Alarm to ac Neutral.

### Alarm 2 (Setpoint) Hook up

- Connect a jumper from ac Line to Relay 2 Common (Terminal 6).
- Connect Relay 2 Normally Open (Terminal 4) to External Alarm ac Line.
- Connect External Alarm to ac Neutral.

## Analog Output Wiring for 4 - 20 mA Current

- Connect Positive Lead to Terminal 11.
- Connect Negative Lead to Terminal 12.

## For 0 -10 Voltage

- Connect Positive Lead to Terminal 10.
- Connect Negative Lead to Terminal 12.

## Using the Configuration Menu

To configure the meter, you use the buttons on the front panel.

To:	Take This Action:
Display the Configuration Menu	Press the <b>MENU</b> button. The first function on the menu, <b>INPE</b> , displays.
Select a submenu function	<ol style="list-style-type: none"> <li>Press <b>MENU</b> until the function you want is shown.</li> <li>Press <b>▶/DEV</b>. The information you can change flashes.</li> </ol>
Select a value for that submenu function	<ol style="list-style-type: none"> <li>Press <b>▲/MAX</b> to display the option you want.</li> <li>Press <b>MENU</b> to store it. <b>StRd</b> quickly flashes, indicating that the selection has been stored in memory. Then the next menu function displays.</li> </ol>
Go back to previous menu function	Press <b>RESET</b> once.
Exit the Configuration Menu	Press <b>RESET</b> twice. The unit displays <b>RSE</b> as it reinitializes. When a numeric value displays, the unit is in run mode. (Optionally, you can press <b>MENU</b> to move through all the menu functions until the unit reinitializes.)

MENU	SUBMENU ▶/DEV	DESCRIPTION
<b>INPE</b>	<b>U.EC, U.EC*, U.J.EC, E.EC</b>	Input
<b>DECP</b>	<b>FFF.F*, FFF.F</b>	Decimal Point
<b>RD.CF</b>	<b>R.1=C, R.1=F*</b>	Reading Configuration
<b>COLR</b>	<b>GRN, RED, AMBR</b>	Display Color
<b>S1.CF</b>	<b>S.1=A*, S.1=B S.2=U*, S.2=L</b>	Setpoint 1 Configuration
<b>S2.CF</b>	<b>S.1=A*, S.1=B S.2=U*, S.2=L</b>	Setpoint 2 Configuration
<b>S1.db</b>	<b>0000*</b>	Setpoint 1, Deadband
<b>S2.db</b>	<b>0000*</b>	Setpoint 2, Deadband
<b>OE.CF</b>	<b>0.1=E*, 0.1=D 0.2=C*, 0.2=P 0.3=A*, 0.3=B 0.4=D, 0.4=R 0.5=F, 0.5=H</b>	Analog Output Configuration
<b>P.bNd</b>	<b>0000</b> shown if 0.3 = P	Proportional Band
<b>M.RSE</b>	<b>0000</b> shown if 0.3 = P	Manual Reset
<b>OS.S.O</b>	<b>Rd 1, OUT 1, Rd 2, OUT 2</b>	Output Scale & Offset
<b>CJ.OF</b>	<b>0000</b>	Cold Junction Offset
<b>LK.CF</b>	<b>R5=E*, R5=D SP=E*, SP=D L3=0*, L3=1</b>	Lockout Configuration
<b>BRT</b>	<b>H.brE, L.brE, H.brE</b>	Display Brightness






 NEW

\* Factory Default Settings.

## Using the Menus

To Change the Thermocouple Type:

- Press **MENU** until the display shows **INPE**
- Press **▶/DEV** to show current thermocouple type:
- Press **▲/MAX** to select the setting from J, K, T or DJ.TC.
- Press **MENU** to store the value.



- Press **RESET** twice to display the current temperature.